


## Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System



**Bio SB**  
BIOSCIENCE FOR THE WORLD

www.biosb.com

### Intended Use

For In Vitro Diagnostic Use.

### Summary and Explanation

The Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System is a 2 step Biotin-Streptavidin-Horseradish Peroxidase Detection System that allows for the demonstration of antigens in formalin-fixed paraffin-embedded tissue, frozen sections, cytosmears, and cell preparations. The increased sensitivity of the Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System allows for rapid staining procedures without compromising the quality of stains.

The Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System is suitable for use with mouse or rabbit primary antibodies. The Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System kits are optimized for use with Bio SB primary antibodies; however, these universal kits could be optimized to work with prediluted and concentrated antibodies from other vendors.

### Presentation

The Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System contains a Peroxidase Blocker, a Link of Biotinylated Anti-Mouse and Anti-Rabbit immunoglobulin, a Streptavidin conjugated to Horseradish Peroxidase, a DAB Buffer, and a DAB Chromogen. All components are buffered with stabilizers and an anti-microbial agent.

Catalog No.	Volume/Qty
BSB 0001S	5 mL Each [kit]
BSB 0001	15 mL Each [kit]
BSB 0001L	15 mL Link Only
BSB 0001H	15 mL Label Only
BSB 0001LH	15 mL Link and Label
BSB 0003	50 mL Each [kit]
BSB 0003L	50 mL Link Only

Catalog No.	Volume/Qty
BSB 0003H	50 mL Label Only
BSB 0003LH	50 mL Link and Label
BSB 0005	100 mL Each [kit]
BSB 0005L	100 mL Link Only
BSB 0005H	100 mL Label Only
BSB 0005LH	100 mL Link and Label
BSB 0007	200 mL Each [kit]

Catalog No.	Volume/Qty
BSB 0007L	200 mL Link Only
BSB 0007H	200 mL Label Only
BSB 0007LH	200 mL Link and Label
BSB 0009	1000 mL Each [kit]
BSB 0009L	1000 mL Link Only
BSB 0009H	1000 mL Label Only
BSB 0009LH	1000 mL Link and Label

**Storage** Store at 2-8°C

### Stability

The Mouse/Rabbit ImmunoDetector DAB HRP Brown Detection System is stable up to the expiration date listed on the product label. Do not use this product after the expiration date listed on the product label. Temperature fluctuations should be avoided. Store appropriately when not in use, and avoid prolonged exposure to room temperature conditions.

### Precautions

- 1 For professional users only. Results should be interpreted by a qualified medical professional.
2. Ensure proper handling procedures are used with reagent. Minimize microbial contamination of reagents.
3. Always wear proper personal protective equipment such as laboratory coat, goggles and gloves when handling reagents.
4. Dispose of unused solution according to local and federal regulations.
5. Do not ingest reagent. If reagent is ingested, seek medical advice immediately.
6. Avoid contact with eyes. If contact occurs, flush with large quantities of water.
7. Follow safety precautions for the heating device used for epitope retrieval (TintoRetriever Pressure Cooker (BSB 7008), TintoRetriever PT Module (BSB 7030 or 7033) or similar).
8. For additional safety information refer to Safety Data Sheet for this product.
9. For complete recommendations for handling biological specimens please refer to the CDC document, "Guidelines for Safe Work Practices in Human and Animal Medical Diagnostic Laboratories" (1).

### Specimen Preparation

**Paraffin sections:** This product can be used on formalin-fixed paraffin-embedded (FFPE) tissue sections. Ensure tissue undergoes appropriate fixation for best results. Pre-treatment of tissues with heat-induced epitope retrieval (HIER) is recommended using Bio SB ImmunoDNA Retriever with Citrate (BSB 0020 - BSB 0023), ImmunoDNA Retriever with EDTA (BSB 0030-BSB 0033). Additionally, TintoDeparaffinator Citrate or EDTA (BSB 0175 - BSB 0178) can be used to deparaffinize, retrieve and hydrate FFPE Tissues. Tissue should remain hydrated using Bio SB Immuno/DNA Washer solutions (BSB 0029 & BSB 0042).

**Frozen sections and cell preparations:** This product can be used for labeling acetone-fixed frozen sections and acetone-fixed cell preparations.

## Preparation of Working Solution

The ImmunoDetector Peroxidase Blocker, ImmunoDetector Link Anti-Mouse/Rabbit and Horseradish Peroxidase Label are ready-to-use working solutions, which do not require further preparation. The DAB Chromogen is concentrated and needs to be diluted with the DAB buffer solution (1 drop chromogen/1 ml buffer). Prepare the working DAB Substrate Chromogen Solution right before use.

## Recommended Protocol

1. Cut and mount 3-5-micron formalin-fixed paraffin-embedded tissues on positive charged slides such as Bio SB Hydrophilic Plus Slides (BSB 7028) or TintoDetector Cap Gap Slides (BSB 7006).
2. Air dry for 2 hours at 58° C.
3. Deparaffinize, dehydrate and rehydrate tissues. Additionally, TintoDeparaffinator Citrate or EDTA (BSB 0175 - BSB 0178) can be used to deparaffinize, retrieve and hydrate FPPE Tissues.
4. Subject tissues to heat induced epitope retrieval (HIER) using a suitable retrieval solution such as ImmunoDNA Retriever with Citrate (BSB 0020-BSB 0023) or EDTA (BSB 0030-BSB 0033).
5. Any of three heating methods may be used:

### a. TintoRetriever Pressure Cooker or Equivalent

Place tissues/slides in a staining dish or coplin jar containing the ImmunoDNA Retriever with Citrate or EDTA or TintoDeparaffinator Citrate or EDTA, and place on trivet in the pressure cooker. Add 1-2 inches of distilled water to the pressure cooker and turn heat to high. Incubate for 15 minutes. Release vapor, open and immediately transfer slides to room temperature.

### b. TintoRetriever PT Module or Water Bath Method

Place tissues/slides in a pre-warmed staining dish or coplin jar containing the ImmunoDNA Retriever with Citrate or EDTA, or TintoDeparaffinator Citrate or EDTA at 95°-99° C. Incubate for 30-60 minutes. Open and immediately transfer slides to room temperature.


### c. Conventional Steamer Method

Place tissues/slides in a pre-warmed staining dish or coplin jar containing the ImmunoDNA Retriever with Citrate or EDTA, or TintoDeparaffinator Citrate or EDTA in a steamer, cover and steam for 30-60 minutes.

6. After heat treatment, transfer slides in ImmunoDNA Retriever with Citrate or EDTA, or in TintoDeparaffinator Citrate or EDTA to room temperature and let stand for 15-20 minutes.
7. For manual staining, perform antibody incubation at ambient temperature. For automated staining methods, perform antibody incubation according to instrument manufacturer's instructions.
8. Wash slides with ImmunoDNA washer or DI water.
9. Continue IHC staining protocol. Wash slides between each step with ImmunoDNA washer solution.

## Abbreviated Immunohistochemical Protocol

Step	ImmunoDetector AP/HRP
Peroxidase/AP Blocker	5 min.
Primary Antibody	30-60 min.
1st Step Detection	10 min.
2nd Step Detection	10 min.
Substrate-Chromogen	5-10 min.
Counterstain / Coverslip	Varies

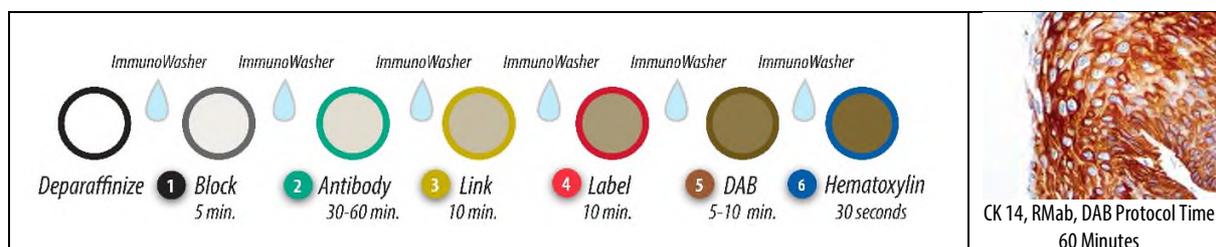

## Mounting Protocol

For detailed instructions using biodegradable permanent mounting media such as XyGreen PermaMounter (BSB 0169-0174) or organic solvent-based resin such as PermaMounter (BSB 0094-0097), refer to PI0174 or PI0097.

## Product Limitations

Due to inherent variability present in immunohistochemical procedures (including fixation time of tissues, dilution factor of antibody, retrieval method utilized and incubation time), optimal performance should be established using positive and negative controls. Results should be interpreted by a qualified medical professional.

## References

1. U.S. Department of Health and Human Services: Centers for Disease Control and Prevention. Guidelines for Safe Work Practices in Human and Animal Medical Diagnostic Laboratories. Supplement / Vol. 61, January 6, 2012.

## Symbol Key / Légende des symboles/Erläuterung der Symbole

<b>EC</b> <b>REP</b>	EMERGO EUROPE Prinsessegracht 20 2514 AP The Hague The Netherlands	Storage Temperature Limites de température Zulässiger Temperaturbereich	Manufacturer Fabricant Hersteller	<b>REF</b>	Catalog Number Référence du catalogue Bestellnummer
<b>IVD</b>	In Vitro Diagnostic Medical Device Dispositif médical de diagnostic in vitro In-Vitro-Diagnostikum	Read Instructions for Use Consulter les instructions d'utilisation Gebrauchsanweisung beachten	Expiration Date Utiliser jusqu'à Verwendbar bis	<b>LOT</b>	Lot Number Code du lot Chargenbezeichnung



69 Santa Felicia Dr., Santa Barbara, CA 93117, USA  
Tel. (805) 692-2768 | Tel. (800) 561-1145 | Fax. (805) 692-2769  
E-mail: sales@biosb.com | Website: www.biosb.com